


Dräger DrugCheck® 3000 Drug Testing Device

Use the Dräger DrugCheck® 3000 to find out within minutes if a person recently consumed certain drugs. The compact and quick saliva (oral fluid) based drug test yields reliable results affordably and easily. The non-invasive drug test kit does not require electricity and can therefore be used anywhere. Now independently verified to comply with AS/NZS 4760:2019.

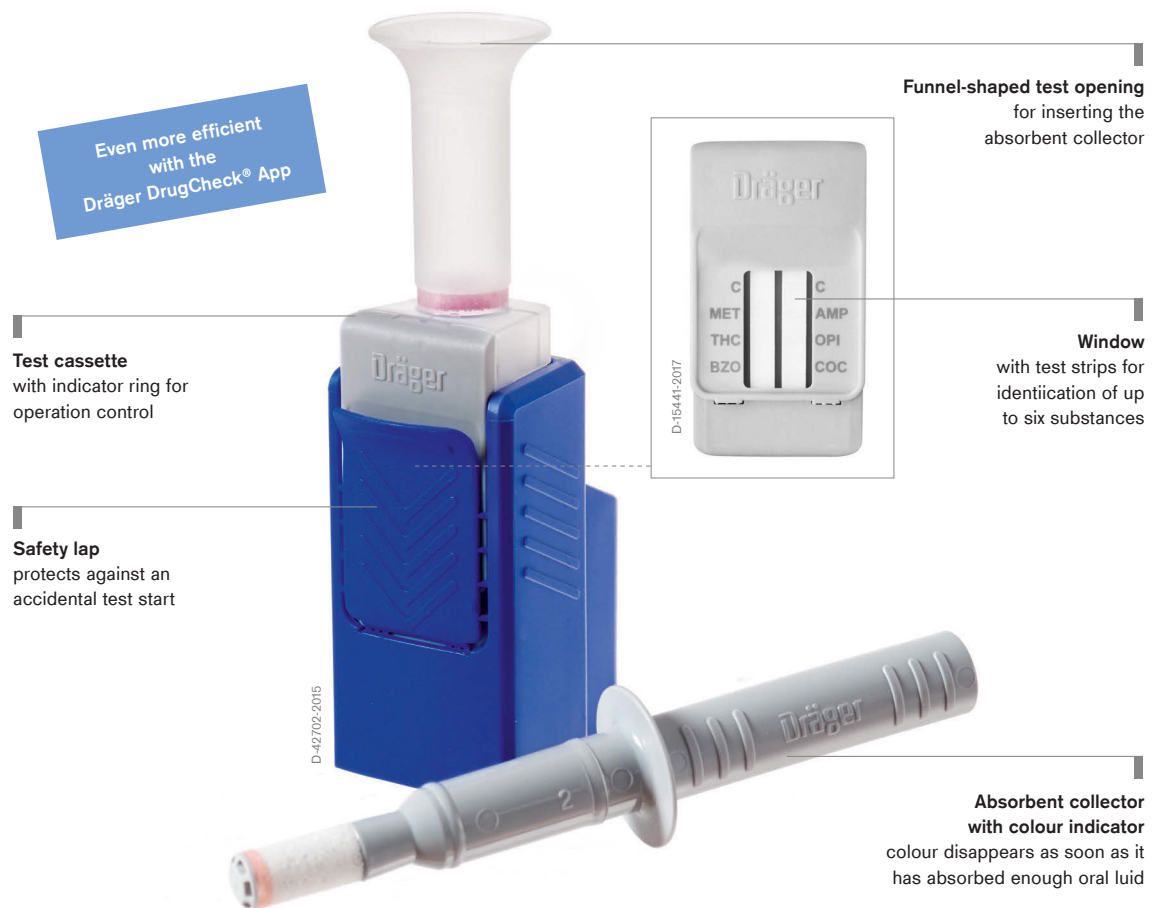

Benefits

DRUG TEST – OBTAIN SAMPLES EASILY AND SAFELY

The Dräger DrugCheck 3000 consists of two components: an absorbent collector for obtaining a saliva sample, and a test cassette for the analysis. The test cassette contains the buffer liquid and a window with two test strips, which displays the control and test lines. The drug test itself is performed in three easy steps: swab the saliva sample, shake the test kit, wait for a brief incubation period, and then start the test. A colour indicator on the swab disappears as soon as it has absorbed enough oral fluid for a test.

As soon as the control lines appear in the window, you can read the results. If the test result is negative, a line will appear alongside the respective substance class (drug). This means that none of the target substance was detected in the sample. If a line fails to appear next to one of the substance classes, then the result for this substance is positive.

FAST AND SENSITIVE DRUG ANALYSIS

Check individuals for up to six substance classes simultaneously with Dräger DrugCheck 3000: cocaine, opiates, oxycodone, amphetamine, methamphetamines/designer drugs (e.g. Ecstasy, MDMA), benzodiazepines (e.g. in prescription medicines) and cannabis (THC). Of all the substance classes listed, cannabis is the drug consumed most frequently and also the most difficult of all compounds to identify (THC = delta-9-tetrahydrocannabinol). This is why the Dräger DrugCheck 3000 was optimised to detect THC, and now offers two measurement options: depending on the chosen waiting time (pre-incubation) of the test there is a fast option with a higher or sensitive option with a lower THC cut-off. The entire drug test only takes 3 – 5 minutes.

UNAMBIGUOUS ON-THE-SPOT DRUG SCREENING

Its compact pocket sized design makes the DrugCheck 3000 easy to transport. It can be made ready for use quickly and easily, and is suitable for flexible use applications such as roadside checks and testing in safety-relevant workplaces. The test kit has no electrical parts, which makes the drug tester safe to use in hazardous areas and even as point-of-care-testing (POCT).

ADDITIONAL BENEFITS

Dräger has decades of experience in alcohol measuring equipment and drug detection methods. For the DrugCheck 3000, Dräger employed the testing principle of the proven Dräger DrugTest® 5000 system, which reliably detects even minute traces of THC. The disposable DrugCheck 3000 test kit cannot be manipulated and is hygienic to use.


Benefits

DRÄGER DRUGCHECK® APP: DRUG DETECTION JUST GOT EVEN MORE CONVENIENT AND EFFICIENT

Scan, test and record the data: mobile data logging on your smartphone is that simple. The new Dräger DrugCheck® App allows you to scan, analyse, log and archive your test results in just a few steps. Video instructions guide you safely through the process of handling the DrugCheck 3000, analysing the test result using your smartphone's camera and storing the result for further use. The results can be clearly logged, together with the personal data of the test subject and tester and information such as the date, time and geographic location. Thanks to the data memory, the test reports generated can be accessed again later.

The encrypted data can be forwarded quickly and easily using a smartphone. This makes it possible to issue recommendations for action based on the test results, even from a remote location. The "Info Area" provides you with more detailed answers, such as on how to conduct a drug test using the DrugCheck 3000. You can download the DrugCheck App for iOS and Android operating systems free of charge from the App Store and Google Play Store. Please note the information on app compatibility with your mobile device.

Details

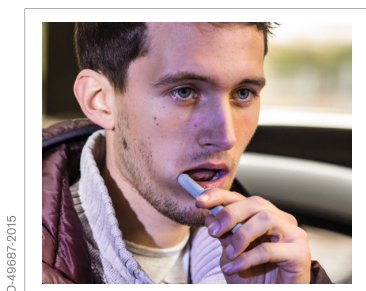

D-49687-2015

1. Take a saliva sample using the sampler



D-49707-2015

2. Insert the sampler into the funnel opening



D-49724-2015

3. Shake the test kit



D-15447-2017

4. Start the test analysis



D-15442-2017

5. Read off the test results



D-27935-2017

6. Get even more efficient drug detection: with the Dräger DrugCheck® App

Services



[DRÄGER DRUGCHECK® APP IN THE APP STORE / GOOGLE PLAY STORE](#)

Scan the QR code to go directly to the download page for the Dräger DrugCheck® App in the App Store / Google Play Store.

Related Products



DRÄGER DRUGTEST® 5000

No pipetting, no drips, no timing: With the Dräger DrugTest® 5000, a drug test is carried out simply and quickly. The collected saliva sample can be analyzed immediately – for accurate results on the spot.



DRÄGER SSK 5000

Ideal for surface drug testing applications, the Dräger SSK 5000 sampling system is quick and easy to use. When used with the Dräger DrugTest® 5000, the sample can be transferred to a test cassette and screened for possible drug contamination. The sample can also be stored and transported for further testing.

Related Products



DRÄGER DCD 5000

Simple, fast and secure detection of intoxicants and drugs:
The Dräger DCD 5000 does not only enable an easy collection of saliva (oral fluid), you can also store the samples and send them to the laboratory for analysis – without the sample being falsified along the way.



DRÄGER SCK

The SCK confirmation set contains two samplers and stabilising components (isopropanol) as well as documentation forms and shipping materials, ensuring a chain of custody through clear documentation and secure shipment of samples to the lab.

Technical Data

Test for detecting drugs in oral fluid

Dimensions (W x H x D)	32 x 111 x 57 mm 1.26 x 4.37 x 2.24 inches
Weight	< 30 g (0,07 lb)
Operating range	Operation: 5 °C to 40 °C (41 °F to 104 °F) at 5 % to 95 % relative humidity
Storage / transportation	4 °C to 25 °C (39 °F to 77 °F)
Time of measurement	Fast measurement: analysis < 3 minutes Sensitive measurement: analysis < 5 minutes
Selecting the measurement mode	Depending on the selected pre-incubation time and the desired THC cut-off fast or more sensitive reading.
Approvals	AS/NZS 4760:2019 verified (STK 6 Oxy variant only)

Ordering Information

Dräger DrugCheck® 3000 Test for detecting drugs in oral fluid	Description	Ordering no.
Dräger DrugCheck® 3000 STK 5	Packaging unit 20 kits	83 25 580
The Dräger DrugCheck® 3000 STK 5 detects the following substances:		
<ul style="list-style-type: none"> - Cocaine (COC) - Opiates (OPI) - Cannabis (THC) - Amphetamines (AMP) - Methamphetamines (MET) 		
Dräger DrugCheck® 3000 STK 6	Packaging unit 20 kits	83 27 960
The Dräger DrugCheck® 3000 STK 6 detects the following substances:		
<ul style="list-style-type: none"> - Cocaine (COC) - Opiates (OPI) - Cannabis (THC) - Amphetamines (AMP) - Methamphetamines (MET) - Benzodiazepines (BZO) 		
Draeger DrugCheck 3000 STK 6 Oxy	Packaging unit 20 kits	3711990
The Draeger DrugCheck 3000 STK 6 Oxy detects the following substances:		
<ul style="list-style-type: none"> - Cocaine (COC) - Opiates (OPI) - Cannabis (THC) - Amphetamines (AMP) - Methamphetamines (MET) - Oxycodone (OXY) 		

AS/NZS 4760:2019
verified.

Notes

Not all products, features, or services are for sale in all countries.
Mentioned Trademarks are only registered in certain countries and not necessarily in the country in which this material is released. Go to www.draeger.com/trademarks to find the current status.

CORPORATE HEADQUARTERS

Drägerwerk AG & Co. KGaA
Moislinger Allee 53–55
23558 Lübeck, Germany

www.draeger.com

AUSTRALIA (HEAD OFFICE)

Draeger Australia Pty. Ltd.
8 Acacia Place
Notting Hill VIC 3168
Tel (Local Toll-free) 1800 372 437
Tel +61 3 9265 5000
customer.service@draeger.com

REGION EUROPE

Dräger Safety AG & Co. KGaA
Revalstraße 1
23560 Lübeck, Germany
Tel +49 451 882 0
Fax +49 451 882 2080
info@draeger.com

REGION MIDDLE EAST, AFRICA

Dräger Safety AG & Co. KGaA
Branch Office
P.O. Box 505108
Dubai, United Arab Emirates
Tel +971 4 4294 600
Fax +971 4 4294 699
contactuae@draeger.com

REGION ASIA PACIFIC

Draeger Singapore Pte. Ltd.
61 Science Park Road
The Galen #04-01
Singapore 117525
Tel +65 6872 9288
Fax +65 6259 0398

**REGION CENTRAL
AND SOUTH AMERICA**

Dräger Indústria e Comércio Ltda.
Al. Pucurui - 51 - Tamboré
06460-100 - Barueri - São Paulo
Tel. +55 (11) 4689-4900
relacionamento@draeger.com

Locate your Regional Sales
Representative at:
www.draeger.com/contact

